

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 010 103

Burettes, 10 ml, straight stopc., PTFE, AS, conf. cert.




Batch: 19-23

Serial:

Measuring Nr. 66475

Batch size: 50

Volume:	10,000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	9,9929 ml	5,9919 ml	1,9976 ml
Deviation:	0,0043 ml	0,0034 ml	0,0033 ml
Precision (CV):	0,0431 %	0,0563 %	0,1675 %

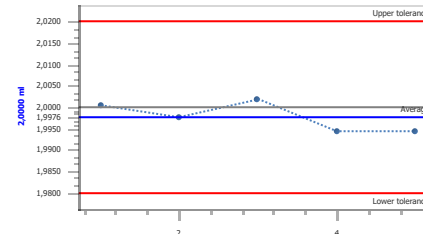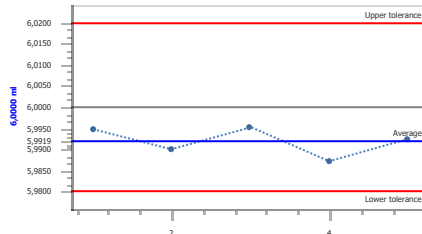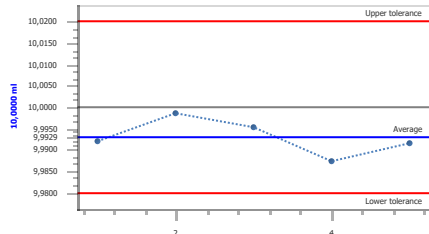

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

27.03.2024

Balance:

Sartorius -
LE244S-OCE

DE-M