

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 010 503

Burettes, 50 ml, str. stopcock, PTFE, AS, conf. cert.




Batch: 09-22

Serial:

Measuring Nr. 59644

Batch size: 99

Volume:	50,000 ml	30,000 ml	10,000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	49,9713 ml	29,9619 ml	9,9904 ml
Deviation:	0,0089 ml	0,0048 ml	0,0054 ml
Precision (CV):	0,0179 %	0,0159 %	0,0544 %

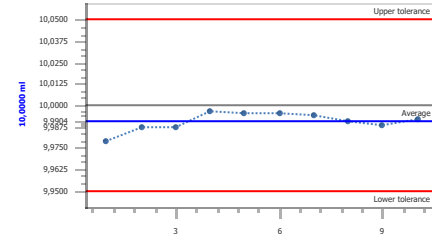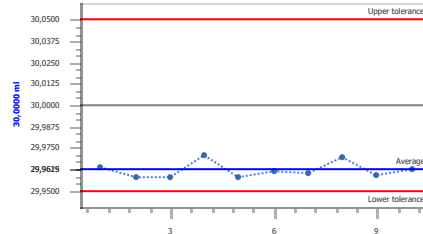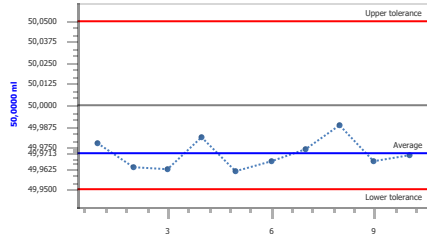

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	10.10.2022
Balance:	Sartorius - MSE224S-0CE -DU

