

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 010 903

**Burettes, 100 ml, straight stopc., PTFE, AS, conf. cert.**




**Batch:** 25-20

**Serial:**

**Measuring Nr.** 58444

**Batch size:** 3

Volume:	100,000 ml	60,000 ml	20,000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	100,0162 ml	60,0345 ml	19,9752 ml
Deviation:	0,0035 ml	0,0115 ml	0,0209 ml
Precision (CV):	0,0035 %	0,0192 %	0,1043 %

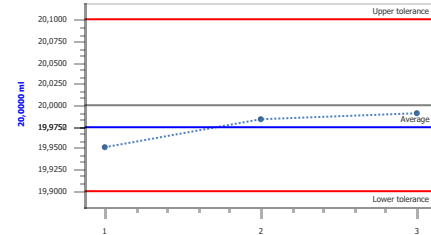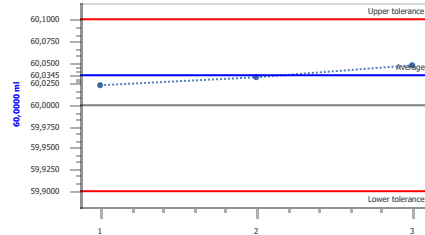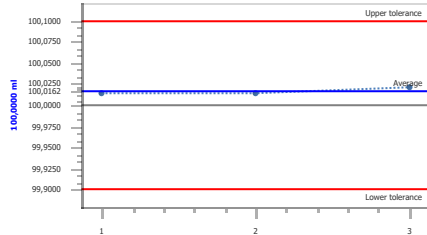

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	7
Date:	30.08.2022
Balance:	Sartorius - LE244S-OCE

