

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 052

Burettes, 5 ml, straight stopc., glass, AS, conf. cert.




Batch: 12-20

Serial:

Measuring Nr. 42634

Batch size: 10

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	5,0059 ml	3,0004 ml	0,9991 ml
Deviation:	0,0013 ml	0,0030 ml	0,0012 ml
Precision (CV):	0,0256 %	0,0994 %	0,1221 %

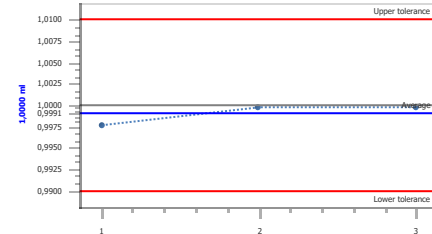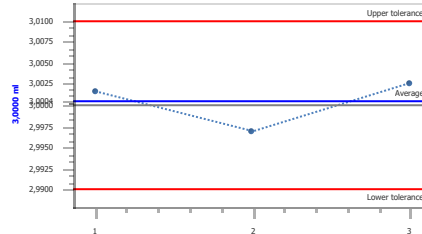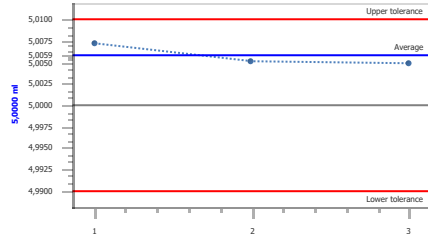

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	18.11.2020
Balance:	Sartorius - MSE224S-0CE -DU

