

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 053

Burettes, 5 ml, str. stopc., PTFE plug, AS, conf. cert.




Batch: 24-16

Serial:

Measuring Nr. 15752

Batch size: 4

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	5,0038 ml	2,9981 ml	1,0001 ml
Deviation:	0,0026 ml	0,0016 ml	0,0028 ml
Precision (CV):	0,0530 %	0,0518 %	0,2780 %

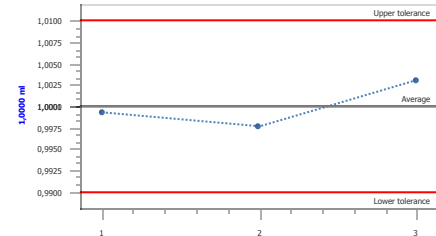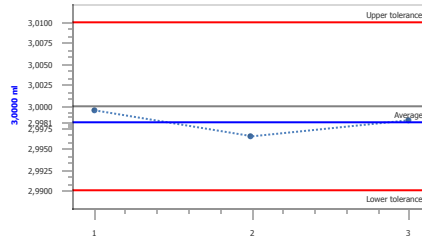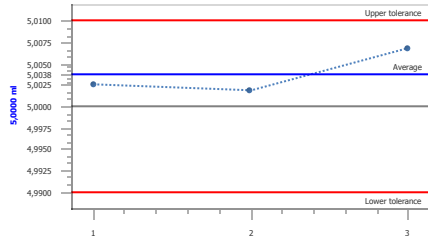

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	16.11.2017
Balance:	Sartorius - LE244S-OCE

