

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 102

Burettes, 10 ml, str. stopcock, glass, AS, conf. cert.




Batch: 23-21

Serial:

Measuring Nr. 53531

Batch size: 10

Volume:	10,000 ml	6,000 ml	2,000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	10,0096 ml	6,0012 ml	1,9978 ml
Deviation:	0,0013 ml	0,0040 ml	0,0030 ml
Precision (CV):	0,0135 %	0,0665 %	0,1506 %

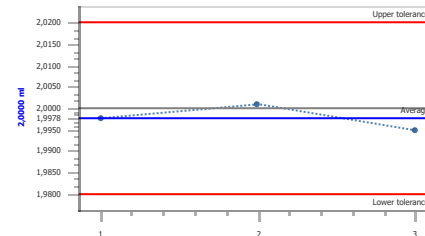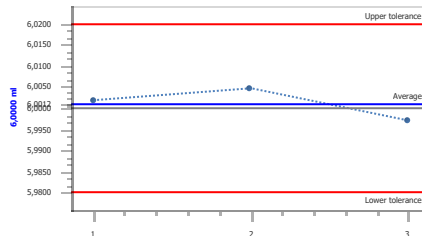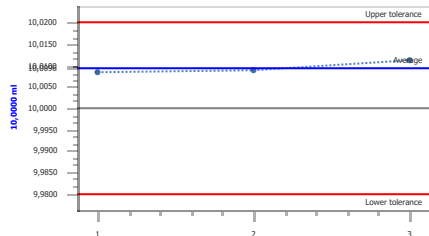

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

7

Date:

24.03.2022

Balance:

Sartorius -
LE244S-OCE

DE-M