

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 103

Burettes, 10 ml, str. stopc., PTFE-plug, AS, conf. cert.




Batch: 26-24

Serial:

Measuring Nr. 68274

Batch size: 100

Volume:	10,000 ml	6,000 ml	2,000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	10,0018 ml	5,9974 ml	1,9974 ml
Deviation:	0,0045 ml	0,0032 ml	0,0021 ml
Precision (CV):	0,0451 %	0,0542 %	0,1073 %

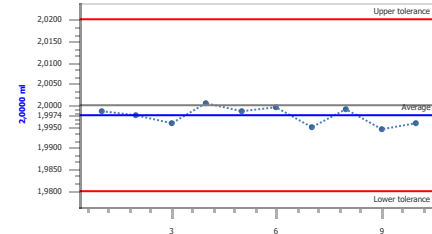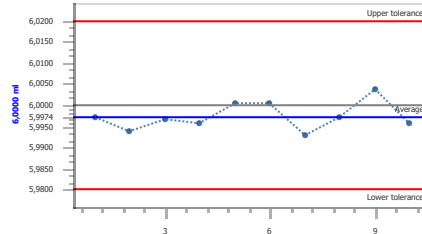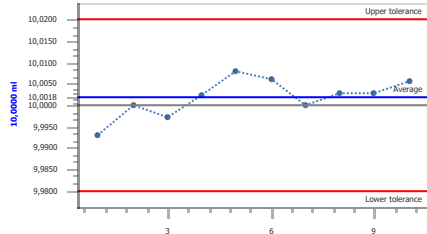

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	77
Date:	31.07.2024
Balance:	Sartorius - LE244S-OCE

