

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 255

Burettes, 25 ml, lat. needle valve, AS, conf. cert.




Batch: 14-19

Serial:

Measuring Nr.: 31763

Batch size: 20

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	25,0117 ml	15,0100 ml	5,0001 ml
Deviation:	0,0044 ml	0,0091 ml	0,0123 ml
Precision (CV):	0,0177 %	0,0607 %	0,2464 %

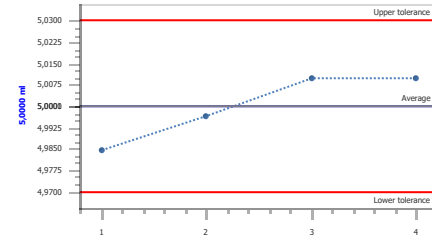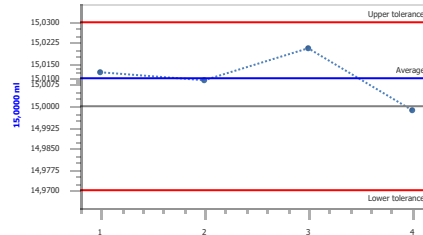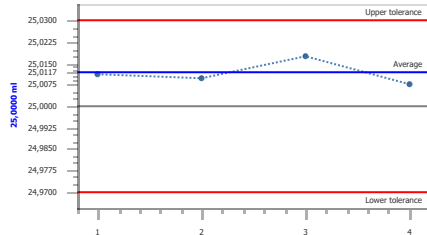

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	18.07.2019
Balance:	Sartorius - LE244S-OCE

