

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 012 255

**Burettes, 25 ml, lat. needle valve, AS, conf. cert.**




**Batch:** 28-20

**Serial:**

**Measuring Nr.:** 41804

**Batch size:** 29

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	25,0134 ml	15,0175 ml	5,0135 ml
Deviation:	0,0053 ml	0,0023 ml	0,0043 ml
Precision (CV):	0,0212 %	0,0155 %	0,0869 %

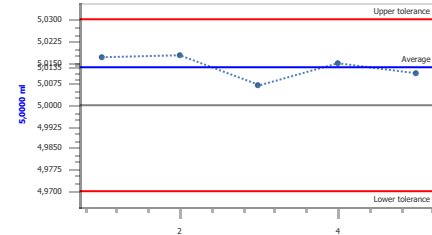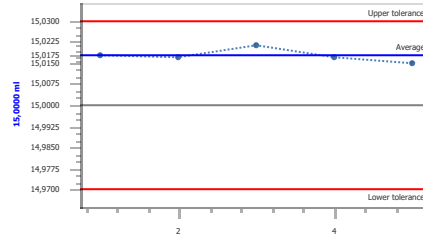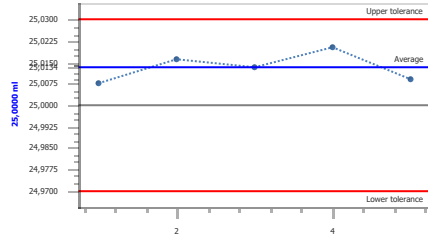

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	7
Date:	28.10.2020
Balance:	Sartorius - LE244S-OCE

