

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 012 255

**Burettes, 25 ml, lat. needle valve, AS, conf. cert.**




**Batch:** 09-22

**Serial:**

**Measuring Nr.** 56873

**Batch size:** 30

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	25,0033 ml	15,0100 ml	5,0074 ml
Deviation:	0,0092 ml	0,0086 ml	0,0053 ml
Precision (CV):	0,0370 %	0,0572 %	0,1064 %

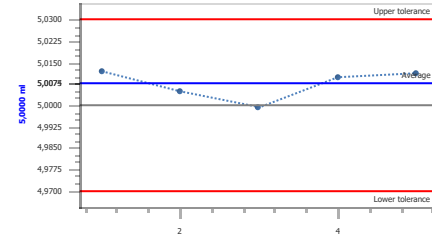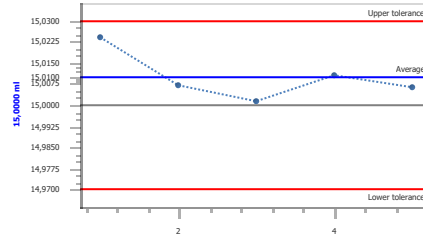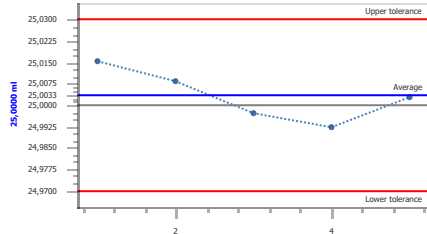

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	7
Date:	30.06.2022
Balance:	Sartorius - LE244S-OCE

