

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 502

Burettes, 50 ml, str. stopc., glass-plug, AS, conf. cert




Batch: 01-19

Serial:

Measuring Nr. 26771

Batch size: 30

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	49,9853 ml	29,9868 ml	9,9948 ml
Deviation:	0,0133 ml	0,0135 ml	0,0146 ml
Precision (CV):	0,0266 %	0,0451 %	0,1460 %

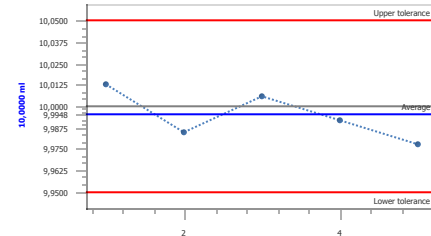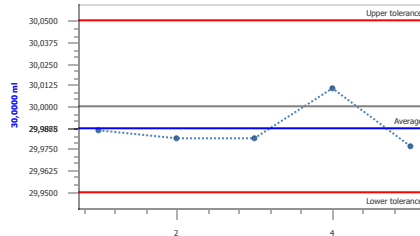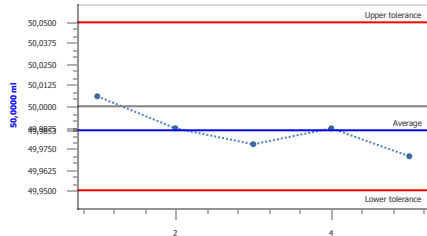

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	14.01.2019
Balance:	Sartorius - LE244S-OCE

