

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 902

Burette, 100 ml, str.stopc., Schellb., AS, conf. cert.




Batch: 13-19

Serial:

Measuring Nr. 33069

Batch size: 5

Volume:	100,000 ml	60,000 ml	20,000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	99,9740 ml	60,0021 ml	20,0120 ml
Deviation:	0,0155 ml	0,0186 ml	0,0132 ml
Precision (CV):	0,0155 %	0,0310 %	0,0660 %

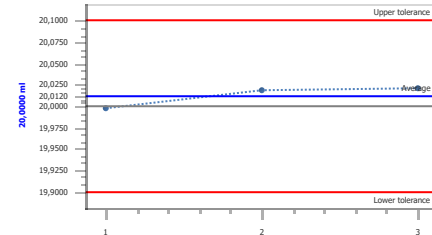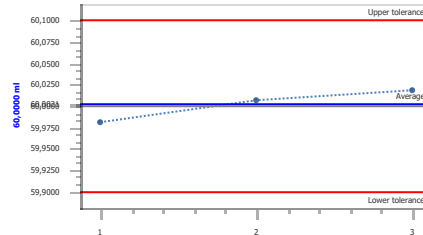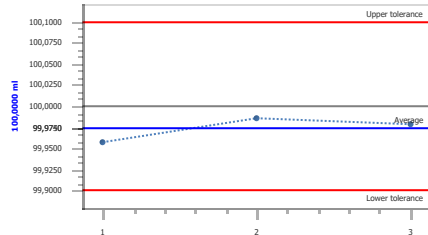

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	17.09.2019
Balance:	Sartorius - LE244S-OCE

