

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 903

Burettes, 100 ml, straight stopcock, AS, conf. cert.




Batch: 41-17

Serial:

Measuring Nr. 15723

Batch size: 10

Volume:	100,000 ml	60,000 ml	20,000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	99,9364 ml	59,9866 ml	20,0051 ml
Deviation:	0,0062 ml	0,0167 ml	0,0091 ml
Precision (CV):	0,0062 %	0,0279 %	0,0456 %

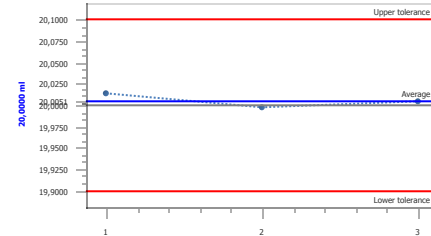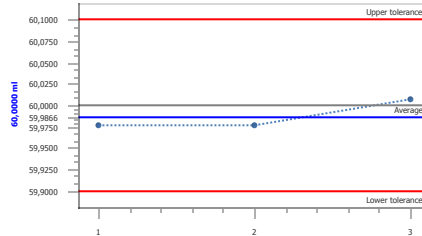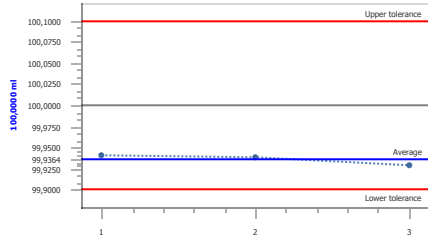

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	15.11.2017
Balance:	Sartorius - LE244S-0CE

DE-M