

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 012 903

**Burettes, 100 ml, straight stopc., PTFE, AS, conf. cert.**




**Batch:** 25-18

**Serial:**

**Measuring Nr.** 24060

**Batch size:** 19

Volume:	100,000 ml	60,000 ml	20,000 ml
<b>Tolerance:</b>	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
<b>Average value:</b>	99,9690 ml	59,9753 ml	19,9999 ml
<b>Deviation:</b>	0,0128 ml	0,0233 ml	0,0211 ml
<b>Precision (CV):</b>	0,0128 %	0,0388 %	0,1053 %

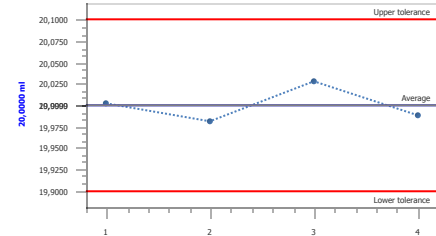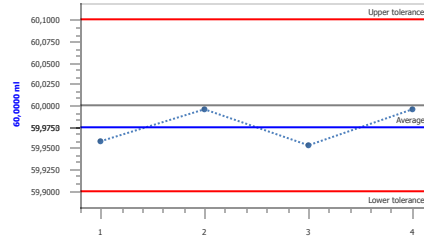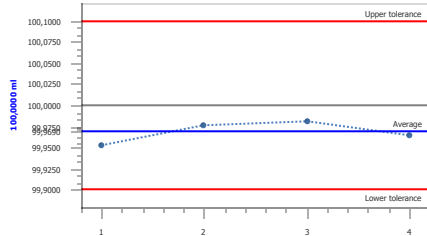

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	9
<b>Date:</b>	14.09.2018
<b>Balance:</b>	Sartorius - LE244S-OCE

