

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 012 905

Burette, 100 ml, lat. stopc., Schellbach, AS, conf. cert.




Batch: 13-19

Serial:

Measuring Nr. 31506

Batch size: 10

Volume:	100,000 ml	60,000 ml	20,000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	99,9451 ml	60,0027 ml	20,0056 ml
Deviation:	0,0152 ml	0,0316 ml	0,0271 ml
Precision (CV):	0,0152 %	0,0526 %	0,1353 %

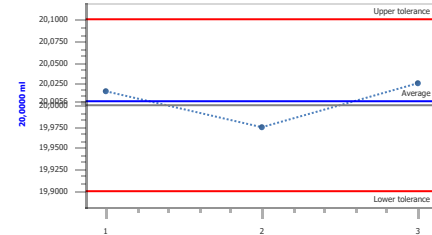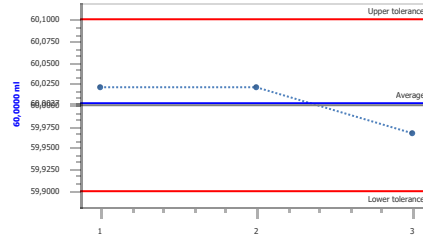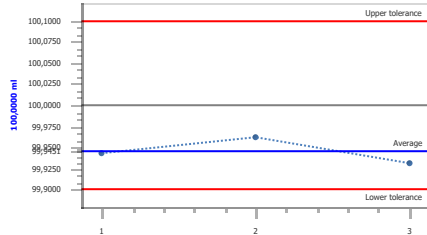

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	15.07.2019
Balance:	Sartorius - LE244S-OCE

