

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 014 102

Burettes, 10 ml, str. stopc., amber glass, AS, conf. cert.




Batch: 43-19

Serial:

Measuring Nr. 34727

Batch size: 10

Volume:	10,0000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	10,0000 ml	5,9947 ml	2,0006 ml
Deviation:	0,0005 ml	0,0011 ml	0,0026 ml
Precision (CV):	0,0052 %	0,0175 %	0,1298 %

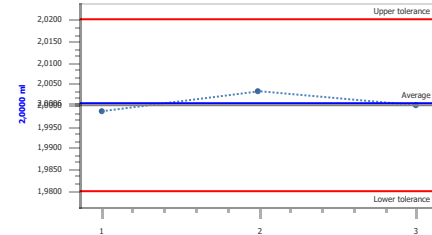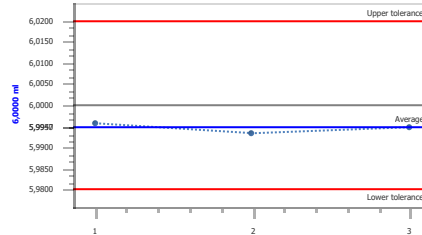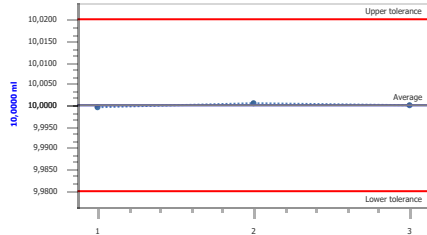

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:

4

Date:

28.11.2019

Balance:

Sartorius -
MSE224S-0CE
-DU

