

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 014 103

**Burettes, 10 ml, str. stopc., amber glass, AS, conf. cert.**




**Batch:** 19-22

**Serial:**

**Measuring Nr.** 65423

**Batch size:** 20

Volume:	10,000 ml	6,0000 ml	2,0000 ml
<b>Tolerance:</b>	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
<b>Average value:</b>	9,9979 ml	5,9903 ml	2,0022 ml
<b>Deviation:</b>	0,0031 ml	0,0024 ml	0,0014 ml
<b>Precision (CV):</b>	0,0313 %	0,0404 %	0,0713 %

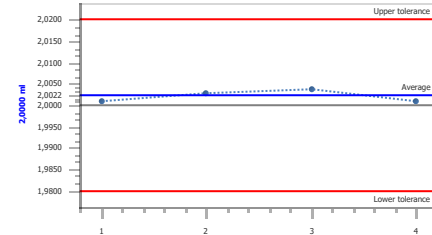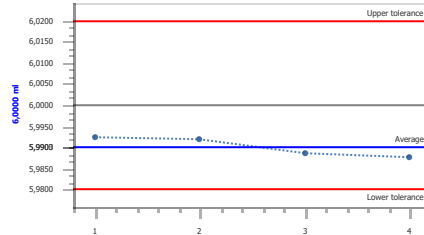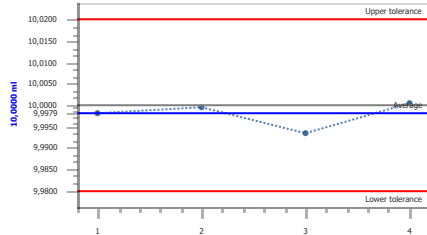

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	05.12.2023
<b>Balance:</b>	Sartorius - LE244S-OCE

