

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 014 503

**Burettes, 50 ml, str. stopc., amber glass, AS, conf. cert.**




**Batch:** 40-17

**Serial:**

**Measuring Nr.** 17468

**Batch size:** 50

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
<b>Tolerance:</b>	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
<b>Average value:</b>	49,9758 ml	29,9756 ml	9,9984 ml
<b>Deviation:</b>	0,0102 ml	0,0102 ml	0,0082 ml
<b>Precision (CV):</b>	0,0204 %	0,0342 %	0,0822 %

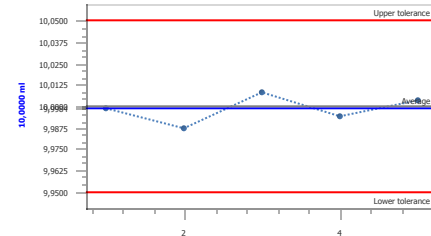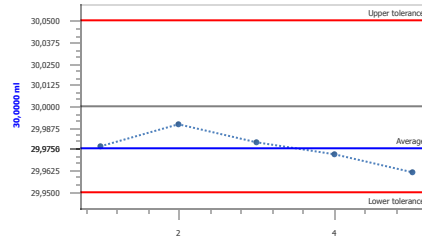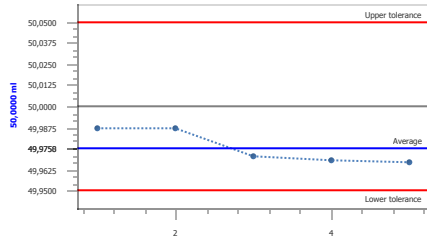

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	4
<b>Date:</b>	24.01.2018
<b>Balance:</b>	Sartorius - LE244S-OCE

DE-M