

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 014 503

Burettes, 50 ml, str. stopc., amber glass, AS, conf. cert.




Batch: 38-17

Serial:

Measuring Nr. 23091

Batch size: 50

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	49,9963 ml	29,9776 ml	10,0009 ml
Deviation:	0,0086 ml	0,0076 ml	0,0037 ml
Precision (CV):	0,0172 %	0,0252 %	0,0371 %

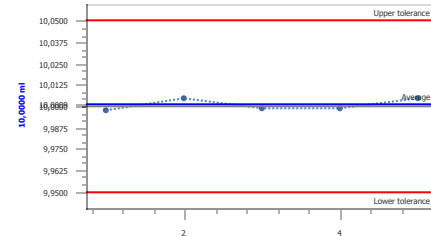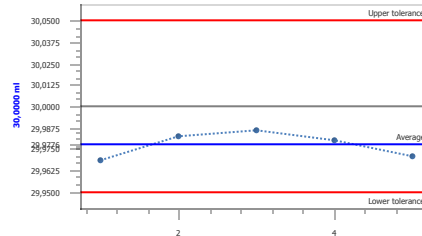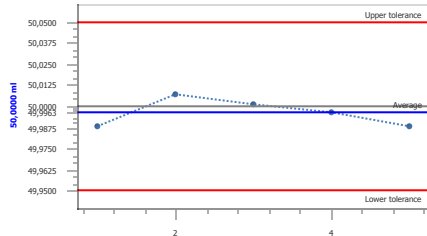

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	07.08.2018
Balance:	Sartorius - LE244S-OCE

