

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 014 503

**Burettes, 50 ml, str. stopc., amber glass, AS, conf. cert.**




**Batch:** 38-17

**Serial:**

**Measuring Nr.** 31806

**Batch size:** 50

| Volume:         | 50,0000 ml  | 30,0000 ml  | 10,0000 ml  |
|-----------------|-------------|-------------|-------------|
| Tolerance:      | ± 0,0500 ml | ± 0,0500 ml | ± 0,0500 ml |
| Average value:  | 50,0135 ml  | 29,9795 ml  | 9,9788 ml   |
| Deviation:      | 0,0080 ml   | 0,0143 ml   | 0,0133 ml   |
| Precision (CV): | 0,0159 %    | 0,0477 %    | 0,1332 %    |

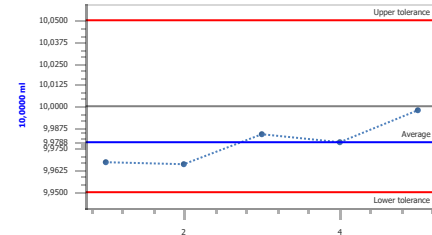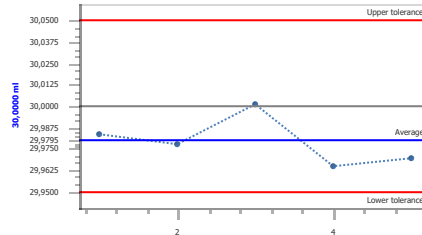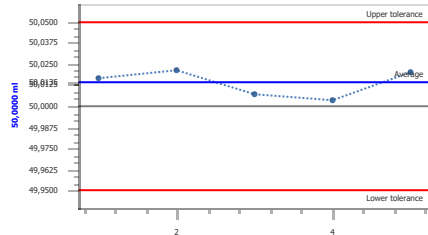

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

|           |                           |
|-----------|---------------------------|
| Operator: | 7                         |
| Date:     | 23.07.2019                |
| Balance:  | Sartorius -<br>LE244S-OCE |

DE-M