

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 014 503

Burettes, 50 ml, str. stopc., amber glass, AS, conf. cert.




Batch: 30-20

Serial:

Measuring Nr. 40165

Batch size: 50

Volume:	50,0000 ml	30,0000 ml	10,0000 ml
Tolerance:	± 0,0500 ml	± 0,0500 ml	± 0,0500 ml
Average value:	50,0113 ml	29,9846 ml	10,0084 ml
Deviation:	0,0159 ml	0,0145 ml	0,0100 ml
Precision (CV):	0,0318 %	0,0483 %	0,1002 %

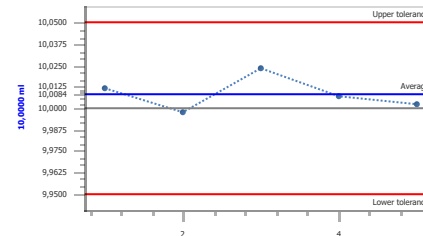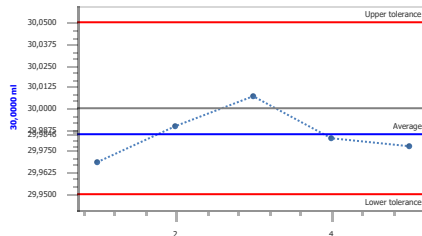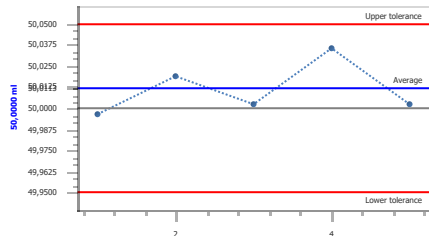

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	16.09.2020
Balance:	Sartorius - LE244S-OCE

