

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 024 257

Burette, 25 ml, str. needle Valve, amber, AS, conf. cert.




Batch: 06-20

Serial:

Measuring Nr. 43478

Batch size: 10

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	24,9942 ml	14,9844 ml	4,9904 ml
Deviation:	0,0072 ml	0,0009 ml	0,0090 ml
Precision (CV):	0,0287 %	0,0060 %	0,1805 %

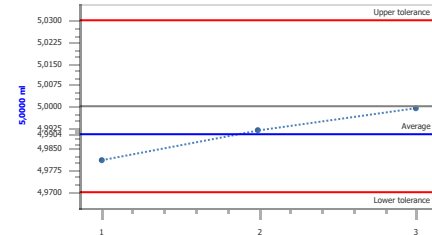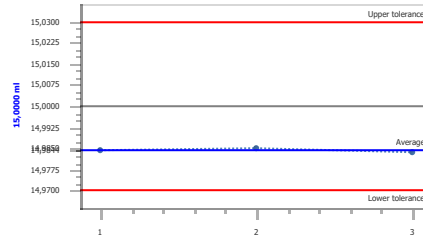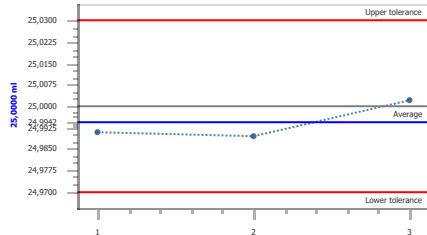

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	09.01.2021
Balance:	Sartorius - LE244S-OCE

DE-M