

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 104

Pellet-burettes, 10 ml, lateral stopcock, AS, conf. cert.




Batch: 33-17

Serial:

Measuring Nr. 19446

Batch size: 10

Volume:	10,000 ml	6,000 ml	2,000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	10,0033 ml	6,0008 ml	1,9991 ml
Deviation:	0,0022 ml	0,0082 ml	0,0038 ml
Precision (CV):	0,0222 %	0,1362 %	0,1902 %

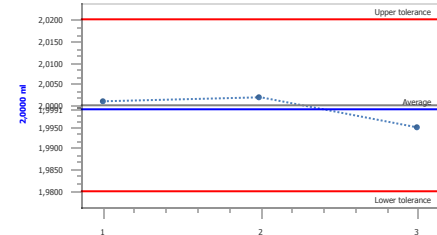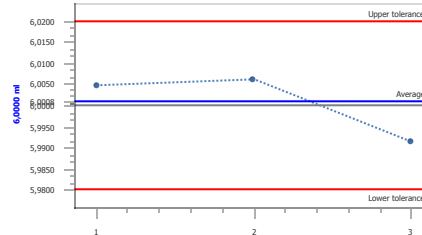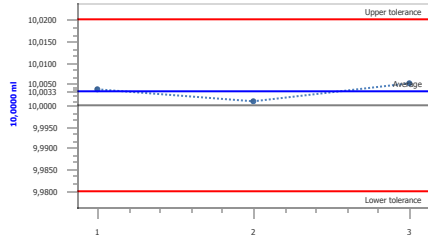

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	04.04.2018
Balance:	Sartorius - LE244S-OCE

DE-M