

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 108

Pellet-burettes, 10 ml, lat. needle valve, AS, conf. cert.




Batch: 07-20

Serial:

Measuring Nr. 38556

Batch size: 30

| Volume: | 10,000 ml | 6,0000 ml | 2,0000 ml |
|------------------------|-------------|-------------|-------------|
| Tolerance: | ± 0,0200 ml | ± 0,0200 ml | ± 0,0200 ml |
| Average value: | 9,9989 ml | 5,9926 ml | 1,9986 ml |
| Deviation: | 0,0060 ml | 0,0049 ml | 0,0045 ml |
| Precision (CV): | 0,0605 % | 0,0820 % | 0,2237 % |

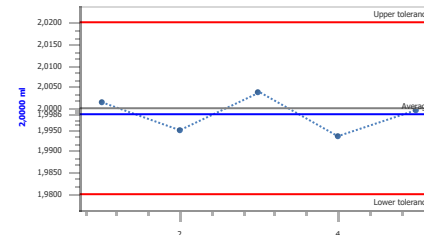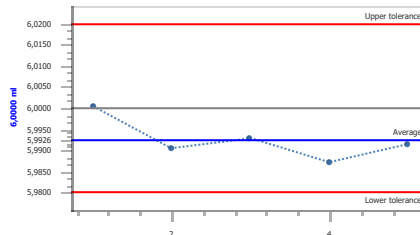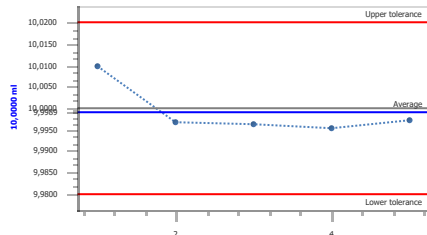

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|------------------|---------------------------|
| Operator: | 9 |
| Date: | 10.06.2020 |
| Balance: | Sartorius - LE244S-OCE |

DE-M