

Certificate of performance



Article: 3 122 108

Pellet-burettes, 10 ml, lat. needle valve, AS, conf. cert.




Batch: 09-21

Serial:

Measuring Nr. 63936

Batch size: 10

Volume:	10,0000 ml	6,0000 ml	2,0000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	10,0165 ml	6,0053 ml	2,0129 ml
Deviation:	0,0015 ml	0,0004 ml	0,0010 ml
Precision (CV):	0,0151 %	0,0072 %	0,0491 %

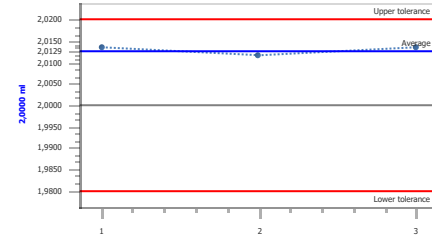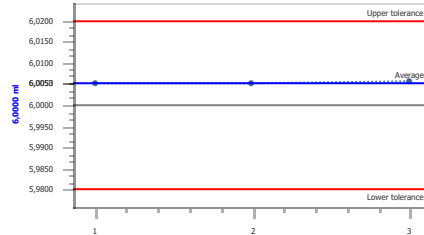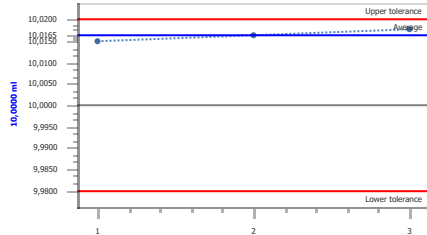

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	14.08.2023
Balance:	Sartorius - LE244S-OCE

