

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 122 258

Pellet-burettes, 25 ml, lat. needle valve, AS, conf. cert.




Batch: 07-20

Serial:

Measuring Nr. 38503

Batch size: 20

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	25,0017 ml	15,0066 ml	4,9981 ml
Deviation:	0,0098 ml	0,0103 ml	0,0087 ml
Precision (CV):	0,0392 %	0,0689 %	0,1734 %

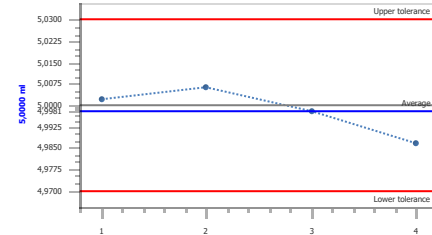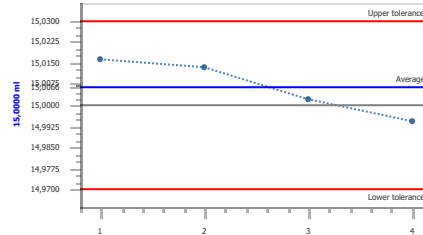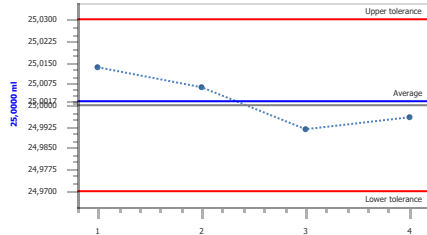

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	09.06.2020
Balance:	Sartorius - LE244S-OCE

