

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 124 256

Pellet-burettes, 25 ml, amber glass, AS, conf. cert.




Batch: 18-19

Serial:

Measuring Nr.: 42593

Batch size: 4

Volume:	25,0000 ml	15,0000 ml	5,0000 ml
Tolerance:	± 0,0300 ml	± 0,0300 ml	± 0,0300 ml
Average value:	25,0065 ml	14,9777 ml	4,9859 ml
Deviation:	0,0089 ml	0,0026 ml	0,0079 ml
Precision (CV):	0,0355 %	0,0176 %	0,1571 %

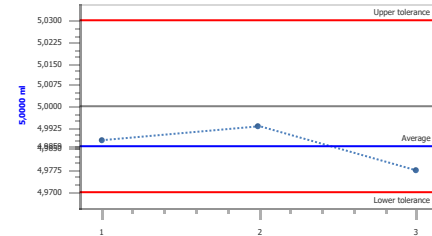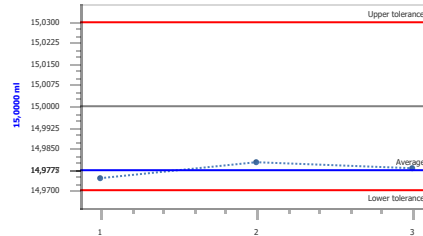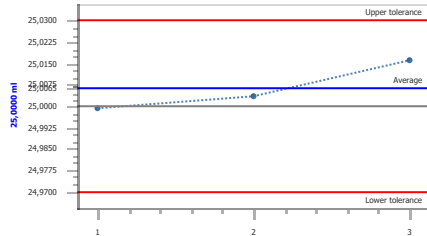

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	17.11.2020
Balance:	Sartorius - MSE224S-0CE -DU

