

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 124 258

Pellet-burettes, 25 ml, amber glass, AS, conf. cert.

Batch: 25-18




Serial:

Measuring Nr.: 26396

Batch size:

6

| Volume: | 25,0000 ml | 15,0000 ml | 5,0000 ml |
|-----------------|-------------|-------------|-------------|
| Tolerance: | ± 0,0300 ml | ± 0,0300 ml | ± 0,0300 ml |
| Average value: | 24,9899 ml | 14,9859 ml | 4,9982 ml |
| Deviation: | 0,0045 ml | 0,0060 ml | 0,0056 ml |
| Precision (CV): | 0,0181 % | 0,0402 % | 0,1127 % |

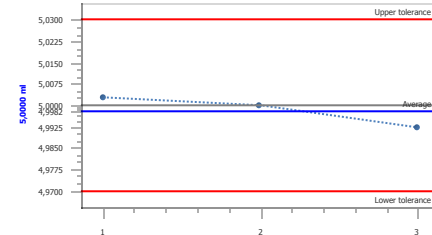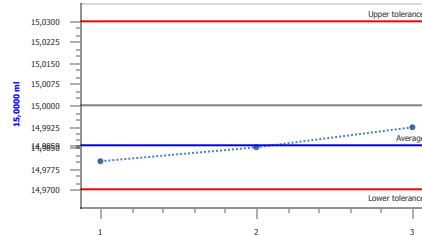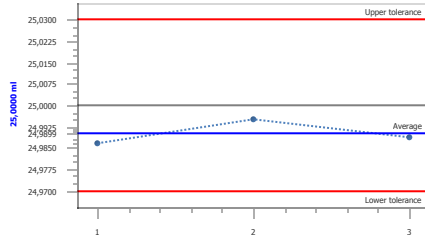

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|-----------|---------------------------|
| Operator: | 9 |
| Date: | 17.12.2018 |
| Balance: | Sartorius - LE244S-OCE |

