

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 152 255

**Univ. automatic burettes, 25 ml, AS, conf. cert.**




**Batch:** 29-20

**Serial:**

**Measuring Nr.:** 47247

**Batch size:** 4

| Volume:         | 25,0000 ml  | 15,0000 ml  | 5,0000 ml   |
|-----------------|-------------|-------------|-------------|
| Tolerance:      | ± 0,0300 ml | ± 0,0300 ml | ± 0,0300 ml |
| Average value:  | 25,0126 ml  | 15,0137 ml  | 5,0117 ml   |
| Deviation:      | 0,0081 ml   | 0,0020 ml   | 0,0018 ml   |
| Precision (CV): | 0,0323 %    | 0,0135 %    | 0,0364 %    |

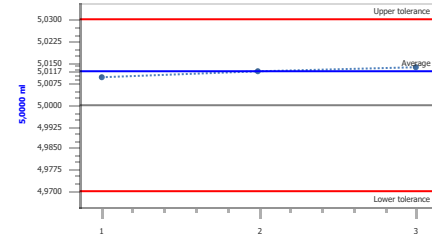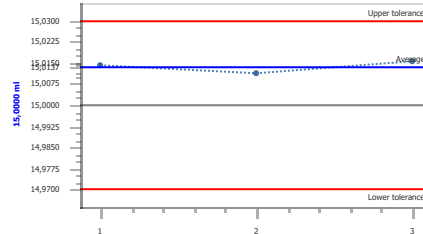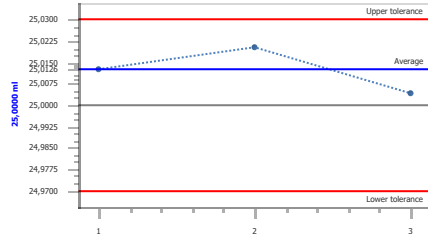

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

|           |                                   |
|-----------|-----------------------------------|
| Operator: | 4                                 |
| Date:     | 09.06.2021                        |
| Balance:  | Sartorius -<br>MSE224S-0CE<br>-DU |

