

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 372 053

**Micro burette, 5 ml, str. stopc., PTFE, AS, conf. cert.**




**Batch:** 40-18

**Serial:**

**Measuring Nr.** 26876

**Batch size:** 6

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	5,0059 ml	3,0010 ml	1,0022 ml
Deviation:	0,0015 ml	0,0016 ml	0,0015 ml
Precision (CV):	0,0294 %	0,0544 %	0,1529 %

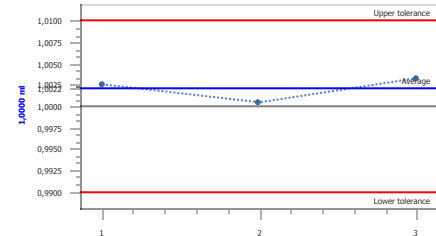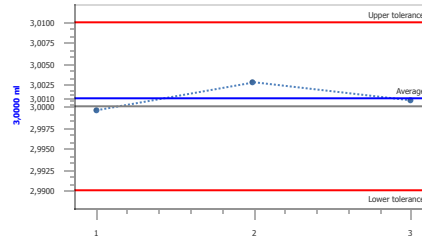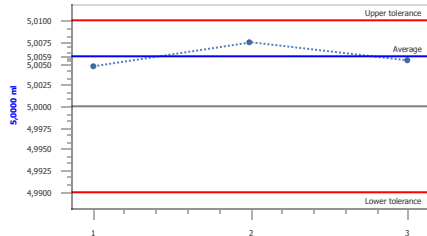

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	4
Date:	17.01.2019
Balance:	Sartorius - LE244S-OCE

DE-M