

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 372 053

Micro burette, 5 ml, str. stopc., PTFE, AS, conf. cert.




Batch: 35-21

Serial:

Measuring Nr. 60072

Batch size: 8

Volume:	5,0000 ml	3,0000 ml	1,0000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	4,9973 ml	2,9977 ml	0,9991 ml
Deviation:	0,0009 ml	0,0008 ml	0,0010 ml
Precision (CV):	0,0185 %	0,0281 %	0,0975 %

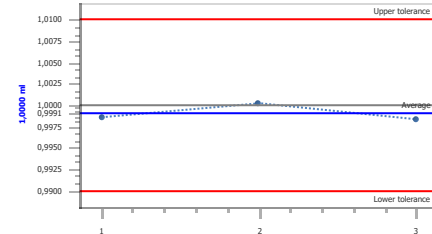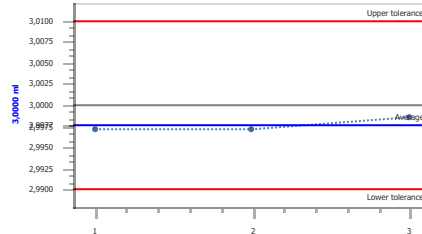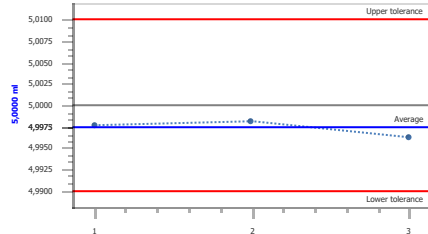

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	77
Date:	04.11.2022
Balance:	Sartorius - LE244S-0CE

