

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 372 103

Micro burette, 10 ml, str.stopc., PTFE, AS, conf. cert.




Batch: 11-22

Serial:

Measuring Nr. 56506

Batch size: 10

Volume:	10,000 ml	6,000 ml	2,000 ml
Tolerance:	± 0,0200 ml	± 0,0200 ml	± 0,0200 ml
Average value:	10,0168 ml	6,0084 ml	1,9978 ml
Deviation:	0,0010 ml	0,0038 ml	0,0027 ml
Precision (CV):	0,0097 %	0,0628 %	0,1375 %

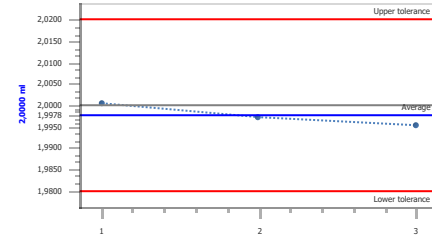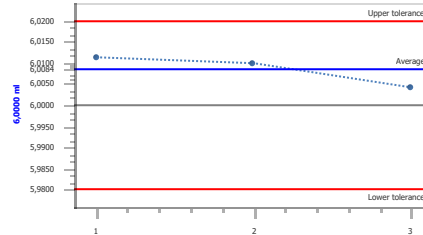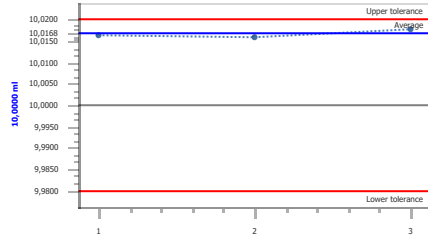

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	07.06.2022
Balance:	Sartorius - LE244S-OCE

