

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 383 025

Micro burettes, 2 ml, lat. needle valve, AS, conf. cert.

Batch: 09-16




Serial:

Measuring Nr. 11812

Batch size:

6

Volume:	2,0000 ml	1,2000 ml	0,4000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	1,9975 ml	1,1976 ml	0,3974 ml
Deviation:	0,0012 ml	0,0016 ml	0,0018 ml
Precision (CV):	0,0603 %	0,1360 %	0,4500 %

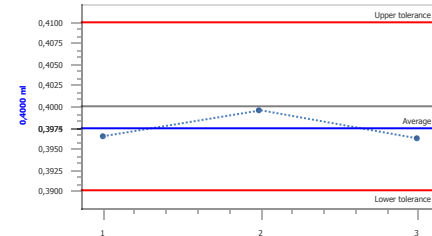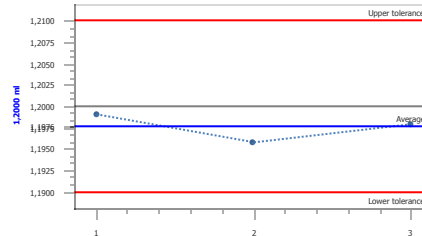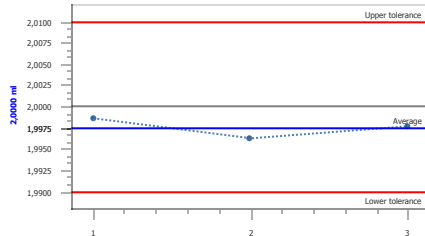

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	04.07.2017
Balance:	Sartorius - LE244S-OCE

