

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 383 025

Micro burettes, 2 ml, lat. needle valve, AS, conf. cert.

Batch: 09-16




Serial:

Measuring Nr. 24538

Batch size:

5

Volume:	2,0000 ml	1,2000 ml	0,4000 ml
Tolerance:	± 0,0100 ml	± 0,0100 ml	± 0,0100 ml
Average value:	2,0013 ml	1,2018 ml	0,3998 ml
Deviation:	0,0038 ml	0,0024 ml	0,0024 ml
Precision (CV):	0,1879 %	0,2010 %	0,5929 %

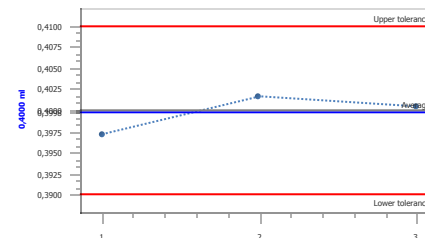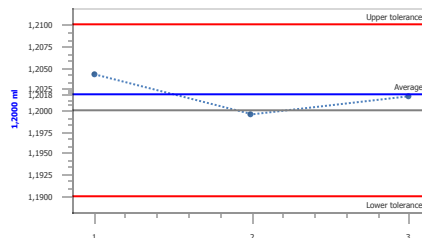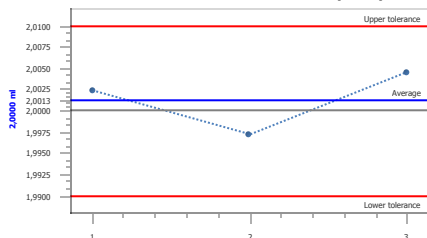

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 385

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	04.10.2018
Balance:	Sartorius - LE244S-OCE

