

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 001 BL

Grad. cylinders, 10:0,2 ml, blue grad, A, conf. cert.




Batch: 27-21

Serial:

Measuring Nr. 47784

Batch size: 280

Volume:	2,0000 ml	6,0000 ml	10,0000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	1,9731 ml	5,9884 ml	10,0102 ml
Deviation:	0,0142 ml	0,0140 ml	0,0207 ml
Precision (CV):	0,7098 %	0,2332 %	0,2073 %

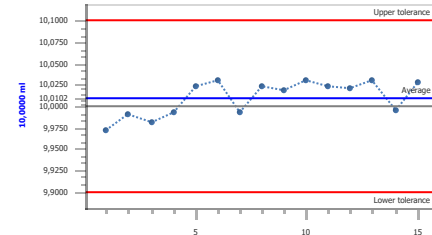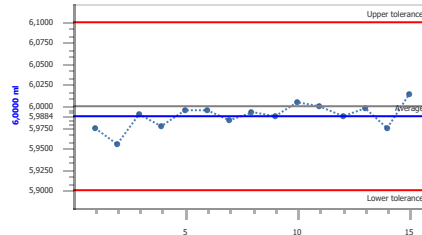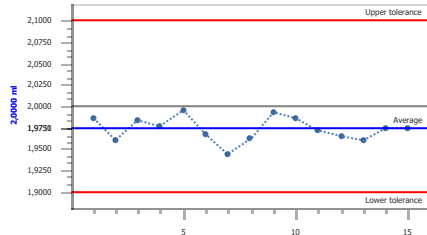

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	07.07.2021
Balance:	Sartorius - LE244S-OCE

