

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 001

**Grad. cylinder, 10:0,2 ml, A, conf.cert.**




**Batch:** 08-25

**Serial:**

**Measuring Nr.** 72006

**Batch size:** 500

Volume:	2,0000 ml	6,0000 ml	10,0000 ml
Tolerance:	± 0,1000 ml	± 0,1000 ml	± 0,1000 ml
Average value:	2,0041 ml	6,0105 ml	10,0110 ml
Deviation:	0,0189 ml	0,0152 ml	0,0152 ml
Precision (CV):	0,9439 %	0,2537 %	0,1516 %

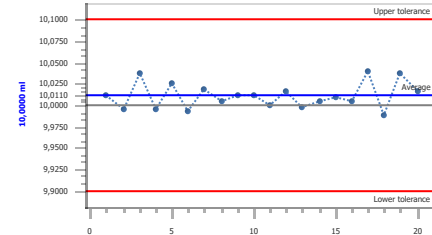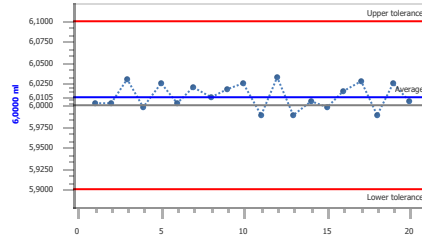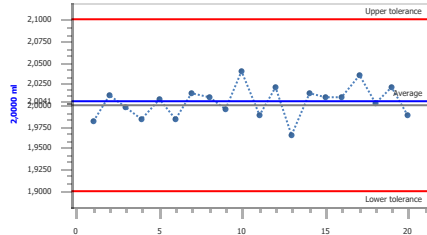

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	7
Date:	19.02.2025
Balance:	Sartorius - LE244S-OCE

DE-M