

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 003 BL

Grad. cylinder, 25:0,5 ml, blue grad., A, conf. cert.




Batch: 36-21

Serial:

Measuring Nr. 48876

Batch size: 500

Volume:	5,0000 ml	15,0000 ml	25,0000 ml
Tolerance:	± 0,2500 ml	± 0,2500 ml	± 0,2500 ml
Average value:	5,0031 ml	15,0002 ml	24,9740 ml
Deviation:	0,0314 ml	0,0269 ml	0,0750 ml
Precision (CV):	0,6281 %	0,1791 %	0,3000 %

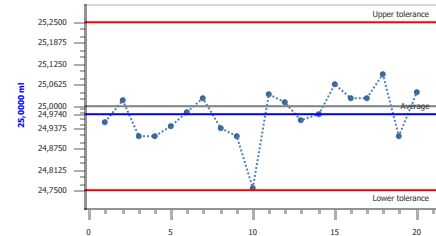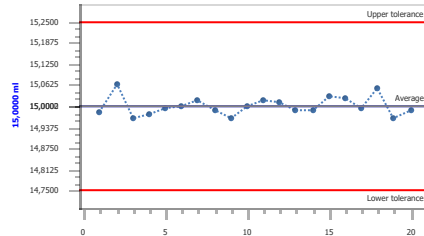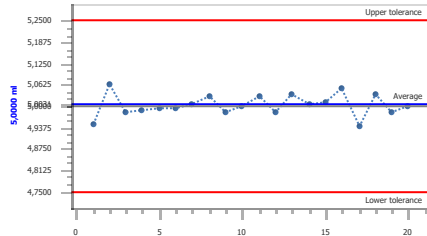

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	15.09.2021
Balance:	Sartorius - LE244S-OCE

