

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 003 BL

Grad. cylinder, 25:0,5 ml, blue grad., A, conf. cert.




Batch: 16-24

Serial:

Measuring Nr. 66737

Batch size: 100

| Volume: | 5,0000 ml | 15,0000 ml | 25,0000 ml |
|-----------------|-------------|-------------|-------------|
| Tolerance: | ± 0,2500 ml | ± 0,2500 ml | ± 0,2500 ml |
| Average value: | 5,0045 ml | 14,9891 ml | 24,9767 ml |
| Deviation: | 0,0290 ml | 0,0394 ml | 0,0327 ml |
| Precision (CV): | 0,5796 % | 0,2624 % | 0,1307 % |

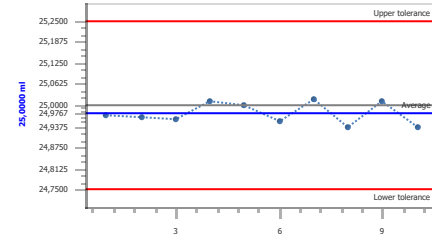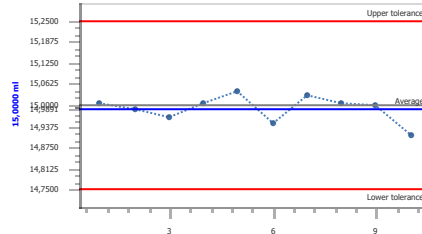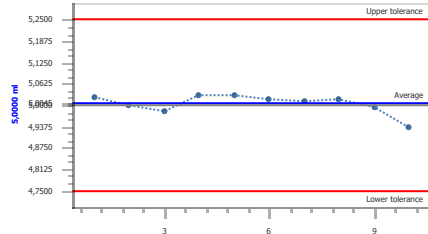

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

| | |
|-----------|---------------------------|
| Operator: | 7 |
| Date: | 11.04.2024 |
| Balance: | Sartorius - LE244S-OCE |

