

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 003 USP

Grad. cyl., 25 : 0,5 ml, USP, A, conf. cert




Batch: 09-22

Serial:

Measuring Nr. 53056

Batch size: 150

Volume:	5,0000 ml	15,0000 ml	25,0000 ml
Tolerance:	± 0,1700 ml	± 0,1700 ml	± 0,1700 ml
Average value:	4,9822 ml	14,9841 ml	24,9821 ml
Deviation:	0,0374 ml	0,0332 ml	0,0329 ml
Precision (CV):	0,7471 %	0,2216 %	0,1315 %

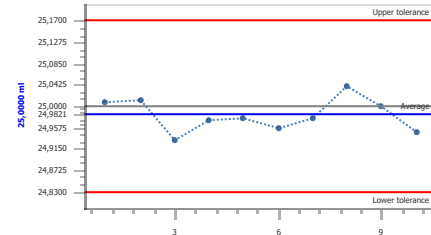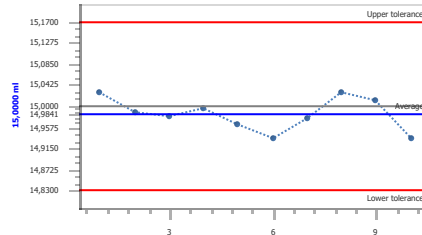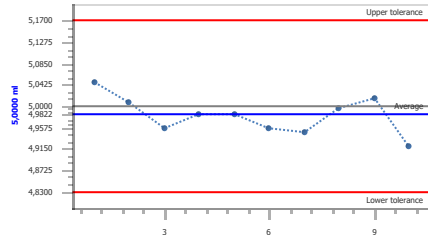

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	15.03.2022
Balance:	Sartorius - LE244S-OCE

