

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 003 USP

**Grad. cyl., 25 : 0,5 ml, USP, A, conf. cert**




**Batch:** 16-24

**Serial:**

**Measuring Nr.** 66739

**Batch size:** 150

Volume:	5,0000 ml	15,0000 ml	25,0000 ml
Tolerance:	± 0,1700 ml	± 0,1700 ml	± 0,1700 ml
Average value:	4,9799 ml	14,9876 ml	24,9847 ml
Deviation:	0,0402 ml	0,0270 ml	0,0184 ml
Precision (CV):	0,8031 %	0,1802 %	0,0736 %

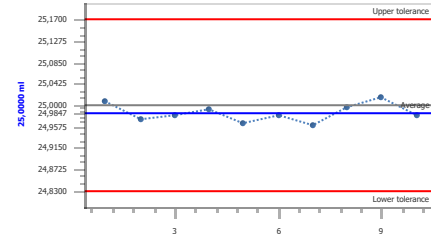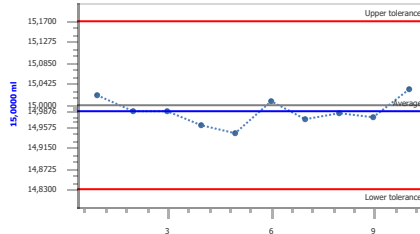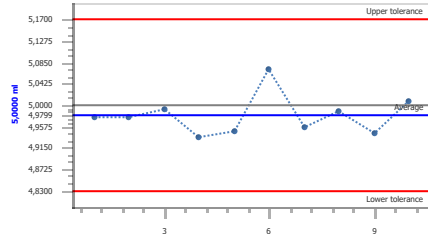

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	7
Date:	12.04.2024
Balance:	Sartorius - LE244S-OCE

