

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 003

Graduated cylinder, 25:0,5 ml, A, conf. cert




Batch: 10-19

Serial:

Measuring Nr. 28272

Batch size: 1050

Volume:	5,0000 ml	15,0000 ml	25,0000 ml
Tolerance:	± 0,2500 ml	± 0,2500 ml	± 0,2500 ml
Average value:	4,9949 ml	15,0096 ml	24,9967 ml
Deviation:	0,0500 ml	0,0442 ml	0,0506 ml
Precision (CV):	0,9995 %	0,2945 %	0,2024 %

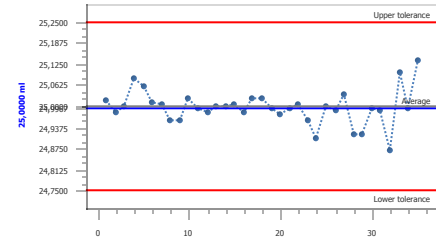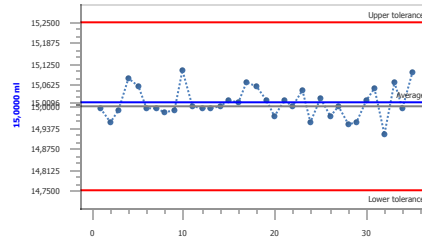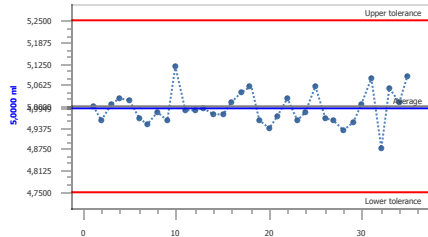

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	13.03.2019
Balance:	Sartorius - LE244S-OCE

