

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 005

Graduated cylinders, 50:1 ml, A, conf. cert.




Batch: 23-22

Serial:

Measuring Nr. 56582

Batch size: 1600

Volume:	10,000 ml	30,000 ml	50,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	10,0448 ml	30,0494 ml	50,0438 ml
Deviation:	0,0700 ml	0,0465 ml	0,0563 ml
Precision (CV):	0,7000 %	0,1551 %	0,1127 %

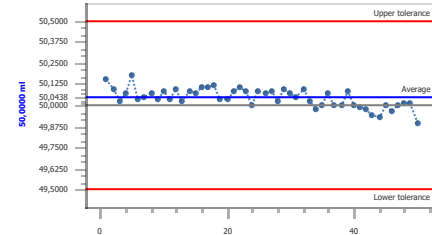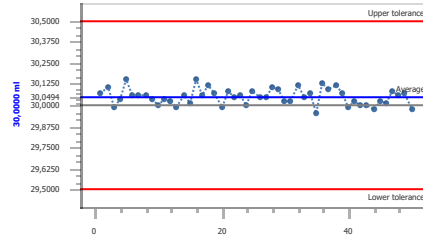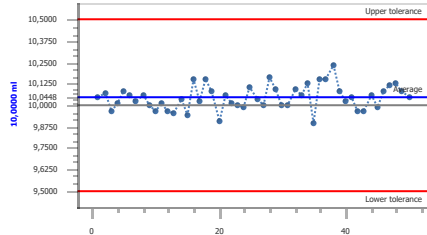

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	20.06.2022
Balance:	Sartorius - MSE224S-0CE -DU

