

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 005

Graduated cylinders, 50:1 ml, A, conf. cert.




Batch: 17-24

Serial:

Measuring Nr. 66992

Batch size: 1200

Volume:	10,000 ml	30,000 ml	50,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	9,9745 ml	29,9953 ml	49,9778 ml
Deviation:	0,0681 ml	0,0578 ml	0,0344 ml
Precision (CV):	0,6805 %	0,1926 %	0,0688 %

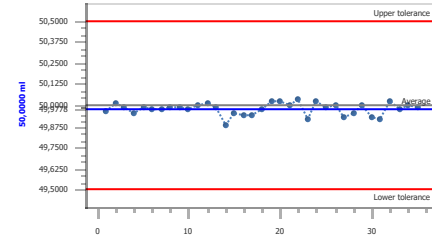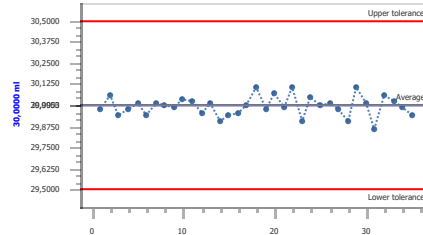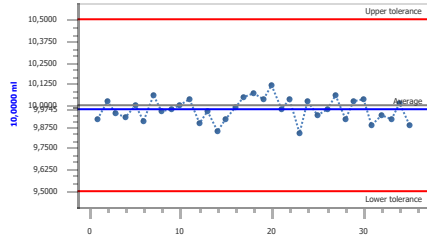

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	29.04.2024
Balance:	Sartorius - LE244S-OCE

