

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 010 BL

Graduated cylinder, 100 ml, blue grad., A, conf. cert.




Batch: 49-17

Serial:

Measuring Nr. 16503

Batch size: 500

Volume:	20,000 ml	60,000 ml	100,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	20,0730 ml	60,0865 ml	100,0816 ml
Deviation:	0,0941 ml	0,0767 ml	0,0598 ml
Precision (CV):	0,4705 %	0,1278 %	0,0598 %

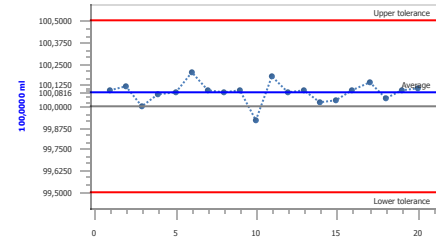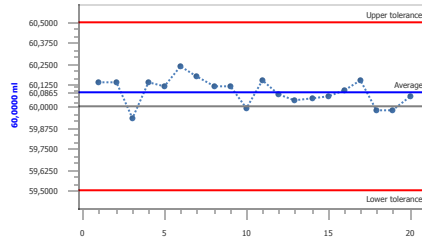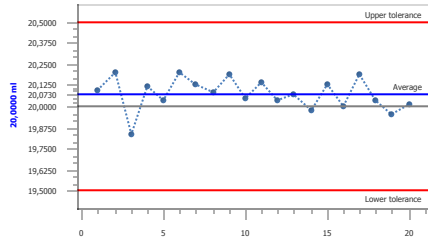

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	9
Date:	16.12.2017
Balance:	Sartorius - LE244S-OCE

