

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 010 BL

Grad. cylinder, 100:1,0 ml, blue grad., A, conf. cert.




Batch: 11-19

Serial:

Measuring Nr. 28362

Batch size: 1200

Volume:	20,000 ml	60,000 ml	100,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	19,8778 ml	59,9033 ml	99,9064 ml
Deviation:	0,1285 ml	0,1073 ml	0,1125 ml
Precision (CV):	0,6427 %	0,1788 %	0,1125 %

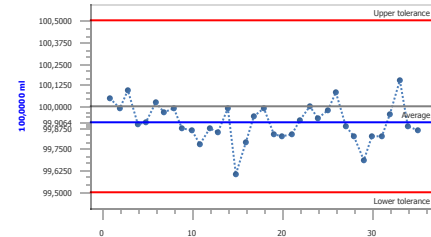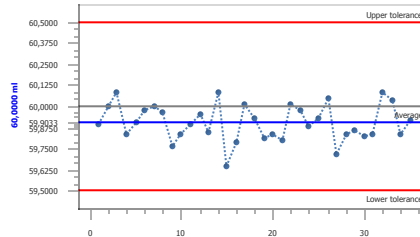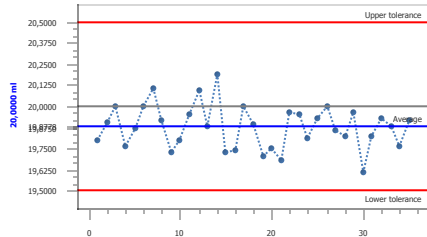

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	0
Date:	19.03.2019
Balance:	Sartorius - LE244S-OCE

