

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 010 BL

**Grad. cylinder, 100:1,0 ml, blue grad., A, conf. cert.**




**Batch:** 23-19

**Serial:**

**Measuring Nr.** 30497

**Batch size:** 500

Volume:	20,0000 ml	60,0000 ml	100,0000 ml
<b>Tolerance:</b>	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
<b>Average value:</b>	19,9077 ml	59,9307 ml	100,0851 ml
<b>Deviation:</b>	0,0556 ml	0,0757 ml	0,0667 ml
<b>Precision (CV):</b>	0,2778 %	0,1261 %	0,0667 %

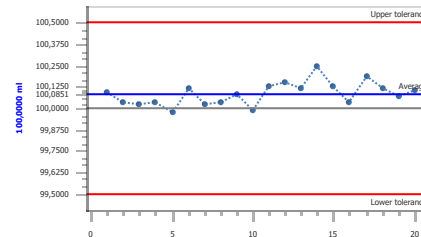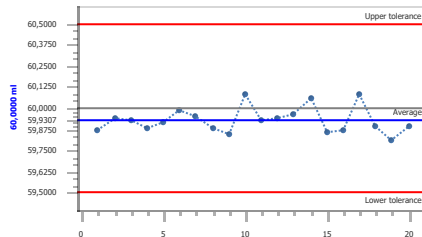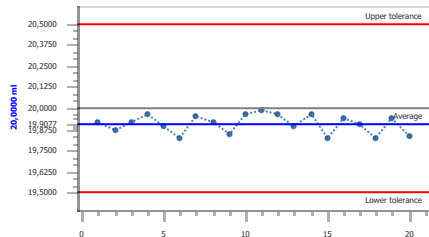

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

<b>Operator:</b>	7
<b>Date:</b>	12.06.2019
<b>Balance:</b>	Sartorius - LE244S-OCE

