

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 010 BL

Grad. cylinder, 100:1,0 ml, blue grad., A, conf. cert.




Batch: 37-20

Serial:

Measuring Nr. 40132

Batch size: 500

Volume:	20,0000 ml	60,0000 ml	100,0000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	19,8853 ml	59,9473 ml	100,1073 ml
Deviation:	0,1290 ml	0,1011 ml	0,0806 ml
Precision (CV):	0,6449 %	0,1685 %	0,0806 %

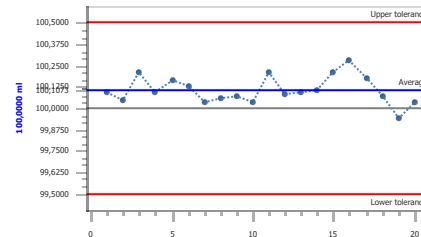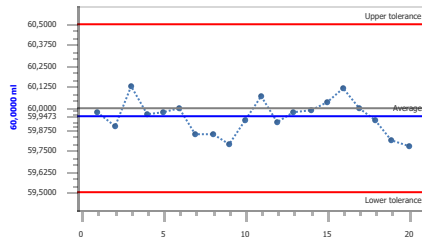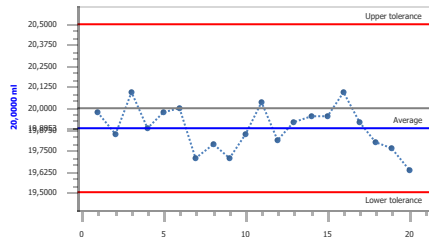

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	16.09.2020
Balance:	Sartorius - LA 1200 S

