

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 010 USP

Graduated cylinders, 100:1 ml, USP, A, conf. cert.




Batch: 01-21

Serial:

Measuring Nr.: 43599

Batch size: 196

Volume:	20,000 ml	60,000 ml	100,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	19,8643 ml	59,9297 ml	100,0026 ml
Deviation:	0,1124 ml	0,0514 ml	0,0683 ml
Precision (CV):	0,5622 %	0,0856 %	0,0683 %

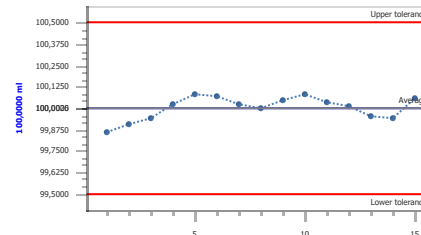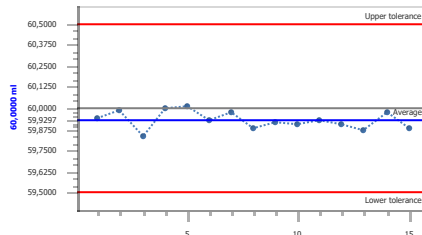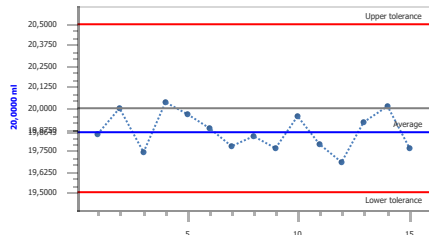

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	7
Date:	18.01.2021
Balance:	Sartorius - LE244S-OCE

