

# Certificate of performance



ISO 9001  
CERTIFIED

**Article:** 3 715 010 USP

**Graduated cylinders, 100:1 ml, USP, A, conf. cert.**




**Batch:** 18-22

**Serial:**

**Measuring Nr.** 55245

**Batch size:** 279

Volume:	20,000 ml	60,000 ml	100,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	20,0147 ml	59,9819 ml	100,0207 ml
Deviation:	0,0782 ml	0,0535 ml	0,0478 ml
Precision (CV):	0,3911 %	0,0891 %	0,0478 %

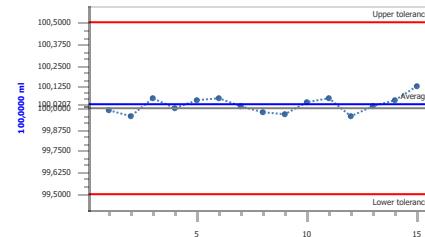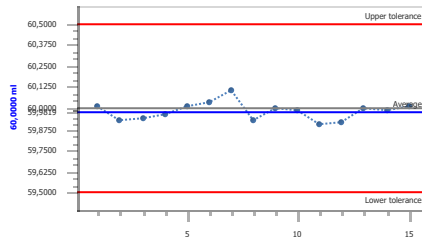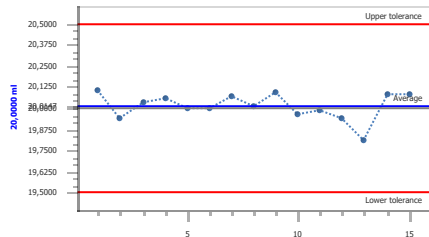

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

**witeg Labortechnik GmbH**

Am Bildacker 16  
97877 Wertheim  
Germany  
+49 (0) 9342 / 9301-0  
info@witeg.de

Operator:	7
Date:	05.05.2022
Balance:	Sartorius - LE244S-OCE

