

Certificate of performance



ISO 9001
CERTIFIED

Article: 3 715 010 USP

Graduated cylinders, 100:1 ml, USP, A, conf. cert.




Batch: 38-22

Serial:

Measuring Nr.: 58996

Batch size: 280

Volume:	20,000 ml	60,000 ml	100,000 ml
Tolerance:	± 0,5000 ml	± 0,5000 ml	± 0,5000 ml
Average value:	19,8847 ml	59,9412 ml	99,9826 ml
Deviation:	0,0931 ml	0,0582 ml	0,0329 ml
Precision (CV):	0,4656 %	0,0970 %	0,0329 %

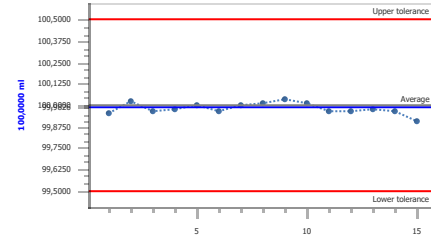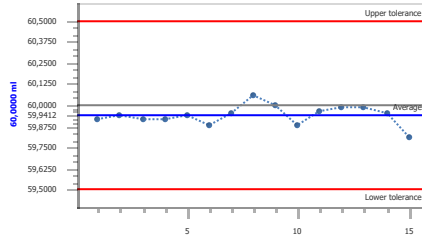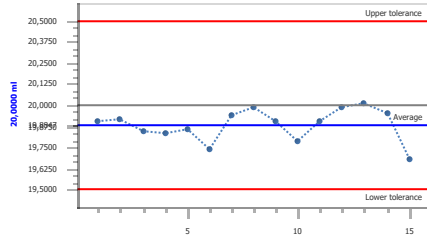

These final test values refer to the delivered nominal volume (max. volume), instrument and liquid (dist. water) at equilibrium with ambient temperature (20 °C). The test was effected according to ISO 4788

witeg Labortechnik GmbH

Am Bildacker 16
97877 Wertheim
Germany
+49 (0) 9342 / 9301-0
info@witeg.de

Operator:	4
Date:	16.09.2022
Balance:	Sartorius - LA 1200 S

